

20–100 mg/L Total Nitrogen, N, Ultra High Range

TNTplus® 828—Method 10208

Scope and application: For water and wastewater.



Test preparation

Test storage

Storage temperature: 15–25 °C (59–77 °F)

pH/Temperature

The pH of the water sample must be between pH 3–12.

The temperature of the water sample and reagents must be between 15–25 °C (59–77 °F).

Before starting

Sodium hydroxide solution A / Oxidant tablet B:

After the addition of reagents A and B, the bottles must be reclosed **immediately**.

Reaction Tubes:

A 20-mm-reaction tube is recommended to be used for **7 times**. After use, clean thoroughly with a brush and tap water. Rinse well with nitrogen-free distilled water and dry.

Turbidity:

Slight turbidities present do not interfere.

Review safety information and expiration date on the package.


Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.


Procedure




1. Preheat the reactor to 120 °C (248 °F).

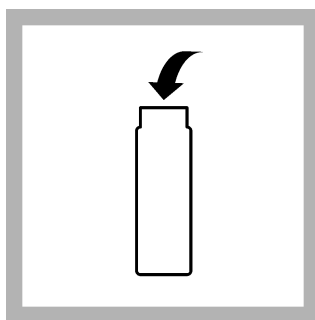


2. Add in quick succession to a dry reaction tube: 0.2 mL sample, 2.3 mL solution A, 1 tablet B.

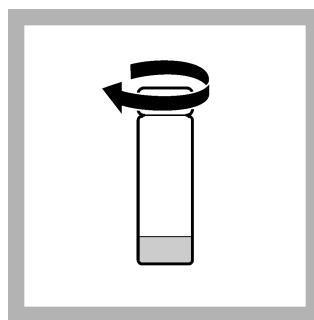


3. Close **immediately** the reaction tube. **Do not** invert.

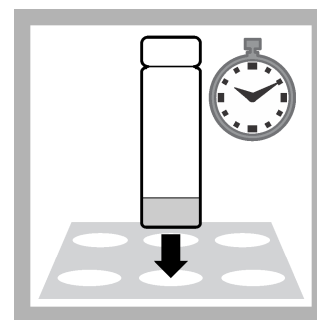


4. Heat for **30 minutes** at 120° C (248° F).

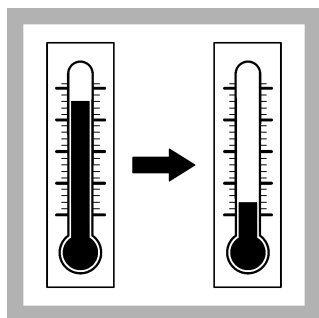


5. Allow to **cool** to room temperature.

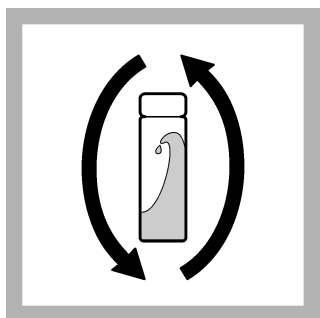


6. Invert a few times.

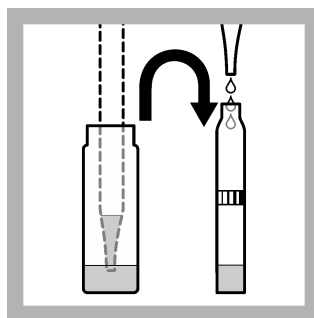


7. **Slowly** pipet into the Cuvette Test: **0.5 mL** of digested sample.

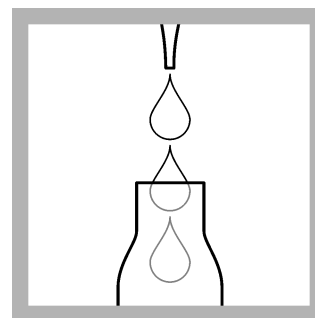


8. **Slowly** pipet **0.2 mL** of solution D.

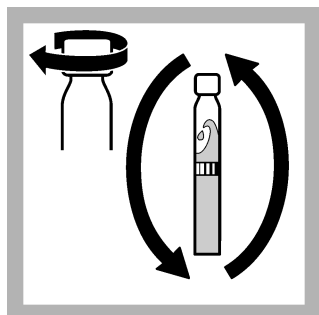

9. Immediately close the cuvette and invert a few times until **no more streaks** can be seen.

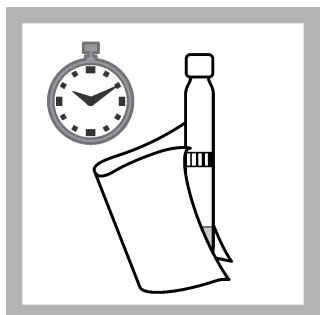

10. After **15 minutes**, thoroughly clean the outside of the cuvette and evaluate.

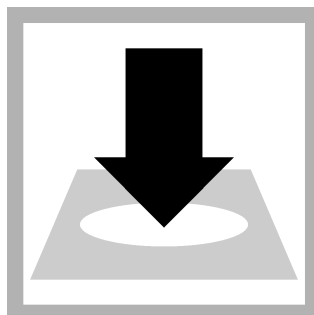

11. Insert the cuvette into the cell holder.
DR 1900: Go to LCK/TNTplus methods. Select the test, push **READ**.

Interferences

A slight pink color may develop during the reaction. This color will not interfere with the analysis.

The ions listed in the table have been individually checked against the given concentrations and do not cause interference. The cumulative effects and the influence of other ions have not been determined.

Low-bias results are expected if the samples contain large amounts of reducing agents.

The measurement results must be subjected to plausibility checks (dilute and/or spike the sample).

Interference level	Interfering substance
5000 mg/L	Cl ⁻
2500 mg/L	COD

Summary of method

Inorganically and organically bonded nitrogen is oxidized to nitrate by digestion with peroxy-disulphate. The nitrate ions react with 2,6-dimethylphenol in a solution of sulphuric and phosphoric acid to form a nitrophenol.

TNT_{plus}[®]



FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:
In the U.S.A. – Call toll-free 800-227-4224
Outside the U.S.A. – Contact the HACH office or distributor serving you.
On the Worldwide Web – www.hach.com; E-mail – techhelp@hach.com

HACH COMPANY
WORLD HEADQUARTERS
Telephone: (970) 669-3050
FAX: (970) 669-2932