

50–2500 mg/L CH₃COOH, (Acetic Acid)

TNTplus®—Method 10240

Scope and application: For digested sludges, activated sludges, process water and food products.



Test preparation

Reagent storage

Storage temperature: 15–25 °C (59–77 °F)

pH/Temperature

The pH of the water sample must be between pH 3–9.

The temperature of the water sample and reagents must be between 15–25 °C (59–77 °F).

Before starting

The analyzed samples must be particle-free and should be filtered (pore size 0.45 µm) if necessary (process waters, activated sludge).

Digested sludge should be centrifuged (10 minutes, 6000 rotations per minute) or filtered. The time taken to obtain the digested sludge water should be as short as possible (< 15 minutes), otherwise the fatty acids may break down, causing a low-bias result to be obtained.


The time taken and the sample preparation procedure up to the execution of the test should be identical for each analysis in order to ensure the best possible quality of the results.

Review safety information and expiration date on the package.


Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.


Procedure

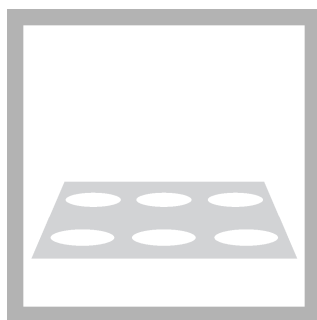


1. Preheat the reactor to 100 °C (212 °F).

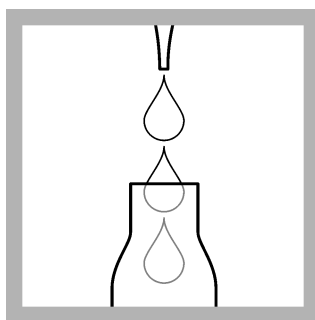


2. Carefully pipet 0.4 mL of solution A.

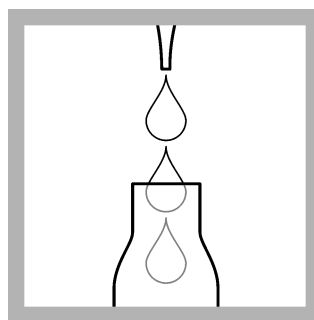


3. Carefully pipet 0.4 mL of sample.

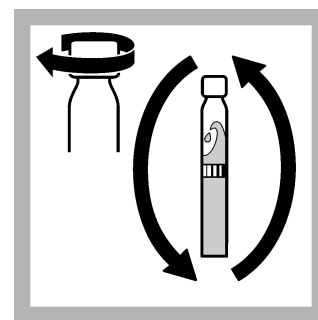


4. Close the vial and invert a few times.

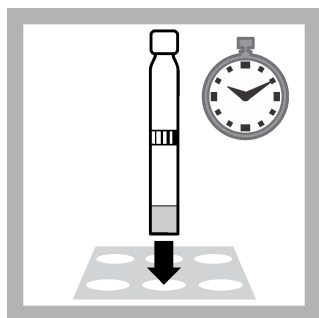


5. Heat in the reactor for **10 minutes** at **100 °C** (212 °F).

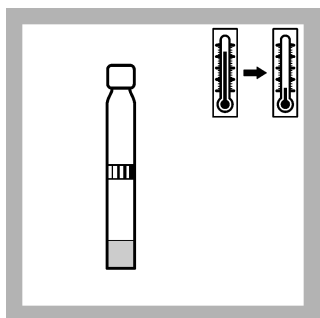


6. Allow to **cool** to room temperature.

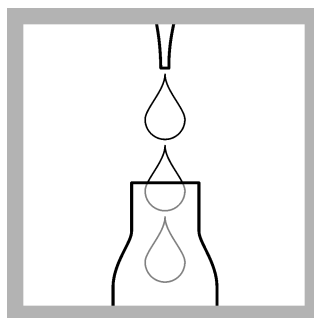


7. Carefully pipet **0.4 mL** of **solution B**.

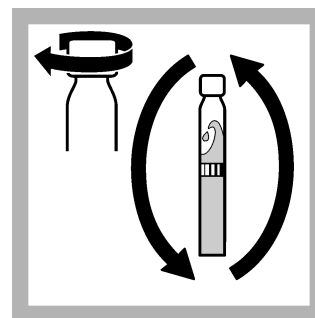


8. Close the vial and invert a few times.

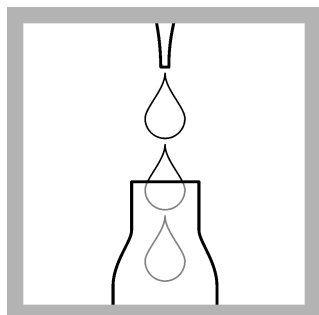


9. Carefully pipet **0.4 mL** of **solution C**.

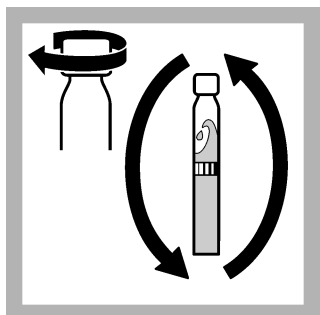


10. Close the vial and invert a few times.

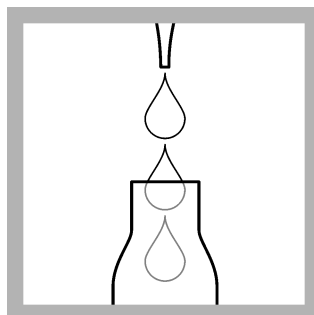


11. Carefully pipet **2.0 mL** of **solution D**.

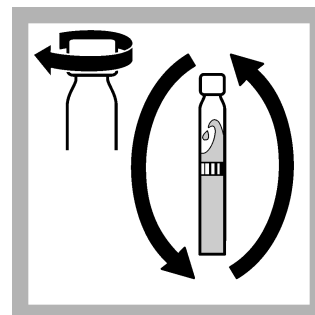

12. Close the vial and invert a few times.

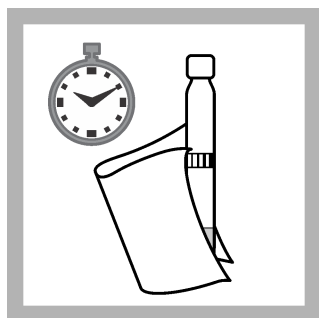

13. After **3 minutes**, thoroughly clean the outside of the vial and evaluate.

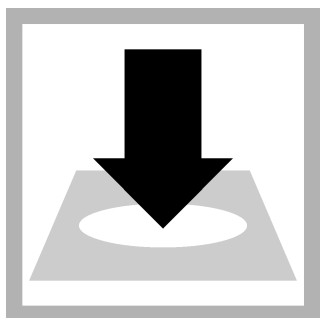

14. Insert the vial into the cell holder.
DR 1900: Go to LCK/TNTplus methods.
Select the test, push **READ**.

Interferences

The ions listed in the table have been individually checked against the given concentrations and do not cause interference.

The cumulative effects and the influence of other ions have not been determined.

The measurement results must be subjected to plausibility checks (dilute and/or spike the sample).

Interference level	Interfering substance
2000 mg/L	Cl^- , SO_4^{2-}
1000 mg/L	Na^+ , K^+ , Ca^{2+} , Mg^{2+}
250 mg/L	NH_4^+

Interference level	Interfering substance
50 mg/L	Al ³⁺ , Cd ²⁺ , Co ²⁺ , Cr ³⁺ , CO ₃ ²⁻ , Cu ²⁺ , I ⁻ , Mn ²⁺ , Mo ²⁺ , NO ₂ ⁻ , Pb ²⁺ , S ²⁻ , Sn ²⁺ , SiO ₂ , SO ₃ ²⁻ , Acetaldehyde, formaldehyde, acetone
25 mg/L	Zn ²⁺
10 mg/L	Ni ²⁺
5 mg/L	Fe ²⁺ , Fe ³⁺ , Cr ⁶⁺

Summary of method

Fatty acids react with diols in an acidic environment, forming fatty acid esters. These are reduced by iron(III) salts to form red coloured complexes, which are evaluated photometrically.

TNT  **plus**®



FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:
 In the U.S.A. – Call toll-free 800-227-4224
 Outside the U.S.A. – Contact the HACH office or distributor serving you.
 On the Worldwide Web – www.hach.com; E-mail – techhelp@hach.com

HACH COMPANY
 WORLD HEADQUARTERS
 Telephone: (970) 669-3050
 FAX: (970) 669-2932